



eISSN 2279-7483

<https://www.pagepressjournals.org/index.php/vl/index>

**Publisher's disclaimer.** E-publishing ahead of print is increasingly important for the rapid dissemination of science. The **Early Access** service lets users access peer-reviewed articles well before print / regular issue publication, significantly reducing the time it takes for critical findings to reach the research community.

These articles are searchable and citable by their DOI (Digital Object Identifier).

**Veins and Lymphatics** is, therefore, e-publishing PDF files of an early version of manuscripts that have undergone a regular peer review and have been accepted for publication, but have not been through the typesetting, pagination and proofreading processes, which may lead to differences between this version and the final one. The final version of the manuscript will then appear in a regular issue of the journal.

E-publishing of this PDF file has been approved by the authors.

*All legal disclaimers applicable to the journal apply to this production process as well.*

Veins and Lymphatics 2024 [online ahead of print]

To cite this article:

Bruno Soggia, Anselmo Pagani, Antonino Proto, et al. Extraction of the Jugular Venous Pulse and carotid profile using a cervical contact plethysmography system. *Veins and Lymphatics*. 2024;13:12664.  
doi:10.4081/vl.2024.12664

 ©The Author(s), 2024  
Licensee PAGEPress, Italy

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

## Extraction of the Jugular Venous Pulse and carotid profile using a cervical contact plethysmography system

Bruno Soggia,<sup>1</sup> Anselmo Pagani,<sup>1</sup> Antonino Proto,<sup>2</sup> Rosa Brancaccio,<sup>3</sup> Angelo Taibi<sup>4</sup>

<sup>1</sup>Department of Translational Medicine and for Romagna, University of Ferrara;

<sup>2</sup>Department of Neuroscience and Rehabilitation, University of Ferrara;

<sup>3</sup>Department of Physics and Astronomy, University of Bologna;

<sup>4</sup>Department of Physics and Earth Sciences, University of Ferrara, Italy

**Corresponding author:** Anselmo Pagani, Department of Translational Medicine and for Romagna, University of Ferrara, Italy.

Tel. +393463087295.

E-mail: [pngnlm@unife.it](mailto:pngnlm@unife.it)

**Key words:** Jugular Venous Pulse, telemedicine, space missions, chronic heart failure, cerebral venous drainage.

**Authors' contributions:** AT, conceptualization, resources, writing – review and editing, supervision, project administration and funding acquisition; BS, methodology, investigation,

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

writing – original draft preparation, review and editing; APa, methodology, investigation, writing – review and editing; APr, data curation, writing – review and editing, visualization; RB, data curation, writing – review and editing. All the authors have read and approved the final version of the manuscript and agreed to be held accountable for all aspects of the work.

**Conflict of interest:** the authors declare no potential conflict of interest.

**Funding:** this work was partially supported by the Italian Space Agency (ASI) under contract n. 2021-1-R.0: Assessment of the cerebral venous outflow in a microgravity environment through the detection of jugular venous pulse oscillations - Drain Brain 2.0.

**Availability of data and materials:** all data generated or analyzed during this study are included in this published article.

**Ethics approval and consent to participate:** the study was approved by the Institutional Ethics Committee.

**Informed consent:** the manuscript does not contain any individual person's data in any form.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

## Abstract

The Jugular Venous Pulse (JVP) is considered a reliable parameter for the assessment of Central Venous Pressure (CVP). Here, the functionality of a cervical contact plethysmography system designed for non-invasive and operator-independent acquisition of the JVP signal, is shown. To validate the signal, it was recorded in supine and sitting positions, together with the reference Electrocardiography (ECG), on 26 healthy subjects. In the supine acquired signal, the characteristic JVP waves (a, c, v) and the negative deflections (x, y) are well recognizable. In the sitting recorded signal, the systolic peak b and the d incisura of the Common Carotid Artery (CCA) waveform are recognized. For each signal, we calculated the Fraction of the Cardiac Cycle (ccf) represented by the time intervals between the JVP peaks and the ECG peaks, in the form:  $\Delta t_{aP}$ ,  $\Delta t_{cR}$ ,  $\Delta t_{xP}$ ,  $\Delta t_{vT}$ ,  $\Delta t_{yV}$ ,  $\Delta t_{vX}$ , and  $\Delta t_{xT}$ . The same was done for the CCA waveform, in the form:  $\Delta t_{bS}$ ,  $\Delta t_{bT}$ ,  $\Delta t_{db}$ ,  $\Delta t_{dS}$ , and  $\Delta t_{dT}$ . This system could mitigate risks and costs associated with central venous catheterization and its potential extends to applications in telemedicine, sports medicine, and space medicine.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

## Introduction

Cardiovascular Diseases (CVDs) currently represent the leading cause of mortality by the World Health Organization (WHO).<sup>1</sup> This necessitates the development of safe, non-invasive, and cost-effective devices for continuous patient monitoring. Such advancements would optimize the availability of monitoring and improve patient care. The Jugular Venous Pulse (JVP) is a reliable marker for pressure changes in the heart throughout the cardiac cycle.<sup>2</sup> The JVP constitutes a periodic waveform characterized by three ascent peaks and three descent peaks, each corresponding to a distinct cardiac event. The initial rise, termed the "a wave," follows the P wave on the Electrocardiogram (ECG) and reflects atrial contraction propelling blood into the ventricle. This ascent is succeeded by the first descent peak, signifying both atrial relaxation and closure of the tricuspid valve, which separates the atrium from the ventricle. Subsequently, the QRS complex on the ECG marks the onset of ventricular contraction. This event is mirrored in the JVP by the "c wave," a rise caused by the bulging of the tricuspid valve as the right ventricle forcefully ejects blood. As pressure decreases following this ejection, a descent peak, the "x descent," is observed on the JVP waveform. Ventricular repolarization, depicted by the T wave on the ECG, coincides with a rise in the JVP waveform known as the "v wave." This rise represents the right atrium filling to its maximum capacity with blood before the tricuspid valve reopens. The opening of the tricuspid valve triggers a final pressure drop, the "y wave," as blood flows rapidly into the ventricle. This completes the cycle, and the JVP waveform repeats.<sup>3</sup> The Common Carotid Artery (CCA) arterial pressure waveform can be divided into distinct phases during the cardiac cycle. The

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

systolic phase encompasses two key components: the upstroke (a wave), characterized by a rise in pressure from the diastolic nadir to the systolic peak (b). This initial rise corresponds to ventricular contraction and subsequent blood ejection into the aorta. Following the peak, a downslope (c) ensues, reflecting the decline in pressure as ventricular relaxation commences and blood flow out of the ventricles begins. A characteristic indentation, known as the aortic notch (d incisura), interrupts this downslope. The aortic notch signifies the closure of the aortic valve, occurring shortly after the onset of diastole. This event marks the end of blood ejection and the return of the pressure waveform to its baseline, the diastolic nadir.

Traditionally, Central Venous Catheterization (CVC) has served as the gold standard for JVP assessment. This invasive procedure necessitates surgical insertion of a catheter into the right internal jugular vein, followed by its advancement towards the right atrium.<sup>4</sup> Due to potential complications, CVC application should be strictly limited to situations of absolute necessity. This study explores a cervical contact plethysmography system as a potential alternative for non-invasive JVP signal acquisition.<sup>5</sup> Ultrasound (US) imaging can be used as an alternative method to assess JVP, but a significant drawback of this technique is its reliance on operator expertise.<sup>6</sup> Employing an automated ultrasound system could overcome this limitation by eliminating operator subjectivity.<sup>7</sup>

## Materials and Methods

### *Experimental protocol*

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

A total of 26 healthy subjects (14 males and 12 females) participated in the study. Their mean age was 25 years ( $\pm 3$  years), mean height was 175 cm ( $\pm 15$  cm), and mean weight was 75 kg ( $\pm 25$  kg). The study was approved by the Local Ethics Committee. All participants undergo anatomical evaluation of the neck's vascular bundle, focusing on the Internal Jugular Vein (IJV) and the CCA, using Doppler ultrasonography. This analysis aims to identify any potential anomalies or pathological conditions that would necessitate subject exclusion, such as IJV entrapment by the omohyoid muscle.<sup>8</sup> For the purpose of validating and precisely identifying the characteristic JVP waves and their corresponding timings, a 3-lead ECG was employed as a reference signal. Following informed consent, subjects autonomously place the device on the neck. Meticulous attention is paid to secure device adherence without compressing surrounding tissues. Compression of superficial cervical venous networks can potentially redistribute venous flow and alter the JVP signal. The plethysmography system placement occurs immediately below the readily identifiable cricoid cartilage (Figure 1). The sensor structure comprises a single-layer dielectric electro active polymer (ElastiSense Sensor Technology, Aabenraa, Denmark). It has non-stretchable zones at both extremities, facilitating secure attachment. The central region functions as the active zone and exhibits high stretchability. The output signal generated by the film corresponds directly to the elongation experienced by this active zone.<sup>9</sup> Subjects are positioned supine and instructed to maintain silence, avoid swallowing, and strive for stable breathing during signal recording. The recording commences with a series of head movements performed by the subject: right and left lateral neck rotations, neck extension, and flexion. These maneuvers serve to calibrate device sensitivity. After 15

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

seconds, subjects execute a maximal inhalation followed by a maximal exhalation. At the end of exhalation, subjects maintain a state of expiratory apnea for 10-15 seconds before resuming normal breathing. This maneuver facilitates the acquisition of a time window free from breathing artifacts. Signal recording lasts for 2 minutes, ensuring the recording of at least four distinct apnea windows. ECG signals are captured synchronously throughout the recording process. The same protocol is repeated with the subject sitting, taking advantage of the shift in venous outflow from the IJVs to the secondary venous pathways, which is associated with complete or partial collapse of the IJVs.<sup>10-14</sup>

### ***Data analysis***

Data processing is performed using Matlab software (MathWorks Inc., Natick, USA). The acquired data were post-processed using MATLAB® software version R2022b. Both the plethysmography traces (JVP and CCA waveform) and the ECG signals underwent noise filtering to emphasize cardiac oscillations. The DC component and breathing artifacts were removed from the signals using a high-pass filter with a cut-off frequency of 0.5 Hz for all signals. Subsequently, a low-pass filter was applied to eliminate high-frequency noise: a cut-off frequency of 4.5 Hz was used for the JVP signal and CCA waveform, and a cut-off frequency of 15 Hz was used for the ECG signal. Regarding the FCC value, we first calculated the cardiac cycle period for each participant. The FCC value was then obtained by dividing each selected time difference by the corresponding cardiac cycle period. Following the generation of final graphs, characteristic JVP peaks and CCA waveform peaks are identified.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

The JVP peaks include the three positive waves (a, c, and v) and the two negative deflections (x and y). The CCA waveform peaks include the systolic peak b and the d incisura. Identification is performed manually by two independent operators for verification purposes. For each cardiac cycle and subject, the Fraction of the Cardiac Cycle (ccf) between JVP peaks and ECG peaks is calculated ( $\Delta taP$ ,  $\Delta tcR$ ,  $\Delta txP$ ,  $\Delta tvT$ ). Additionally, time intervals between JVP peaks ( $\Delta tvy$ ,  $\Delta txv$ ,  $\Delta tax$ ) are also calculated for data analysis (Figure 2). Similarly, time intervals between CCA peaks ( $\Delta tdb$ ), and between CCA peaks and ECG peaks ( $\Delta tdT$ ,  $\Delta tdS$ ,  $\Delta tbT$ ,  $\Delta tbS$ ) were calculated (Figure 3).

## Results

### *Signal shape*

The shape of signals recorded in supine and sitting positions differs markedly (Figure 4A, B). In the acquired tests, the signals of interest exhibited a faithful correspondence to the JVP and the CCA waveform. All characteristic peaks were observed, including the positive deflections a, c, and v, as well as the negative deflections x and y. Notably, peak a consistently occurred subsequent to peak P of the ECG. Peak c was uniquely present during the systolic phase. Finally, peak v and the negative deflections x and y coincided with the T wave. It was possible to identify the b and d peaks of the CCA. It is noteworthy that peak b occurs during the systolic phase, whereas d incisura manifests within the diastolic phase.

### *Signal timing*

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

The ccf of each cardiac cycle and for each subject were calculated, after which the mean value and standard deviation of ccf among all subjects were calculated. The data analysis confirmed the periodicity of the waveforms. What emerges is that, for all of the parameters observed and investigated, except for the  $\Delta tbT$ , the values of the Coefficient of Variations (COV) are below 39%. From this it can be deduced how the mean values ( $\mu$ ) fairly closely represent the values of the observations. In this way it was possible to identify a temporal correlation between the ECG and the JVP, in agreement with what is found in the literature.<sup>15</sup> The results are summarized in Table 1.

## Discussion

This study investigated the feasibility of extracting the JVP waveform from the neck using a cervical contact plethysmography system. The JVP signals were acquired from 26 participants in supine position. Consequently, the data analysis parameters identified herein may contribute to the further development of this system and facilitate comparisons with alternative methods. Adherence to the experimental protocol proved slightly challenging in a subset of participants, particularly those with a higher Body Mass Index (BMI). This difficulty stemmed from limitations in both achieving optimal sensor positioning and maintaining the required apneic state. Future advancements in device development will focus on two key areas. First, further validation will be conducted by comparing the device's JVP extraction capabilities with established methods.<sup>16-19</sup> Second, JVP signal acquisition will necessitate synchronization with both the arterial signal and the ECG. This study establishes, for the first time, the key attributes

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

of a novel cervical contact plethysmography system for JVP signal acquisition, advancing the state-of-the-art in JVP recording techniques. The proposed method offers a user-friendly and cost-effective solution for non-invasive JVP measurement from the neck. It eliminates the need for expensive equipment or complex infrastructure, unlike alternative approaches. Furthermore, the ease of sensor placement around the neck allows for self-application by the subject, thus increasing user comfort and eliminating the requirement for specialized personnel during JVP assessment. These findings hold significant promise for reducing the risks associated with central venous line catheterization, potentially impacting future CVD clinical diagnosis.<sup>20</sup>

## Conclusions

The aim of the study was to validate the JVP signal acquired with the cervical contact plethysmography system. Data analysis from 26 participants identified parameters to inform further system development and comparisons with existing methods. Manual annotation of characteristic a, c, and v waves in the JVP signals, referenced to the ECG, was performed to validate both the observability of JVP waveforms through the device and the feasibility of the proposed method. The calculated time intervals between these key features corroborated the validity of the novel JVP signals and their agreement with established literature, it can be seen that the calculated COV values for ccf are below the 50% cut-off value, as in the article presented by Zamboni *et al.* where JVP was extracted with US.<sup>7</sup> Future directions will focus on system validation against established methods and synchronizing JVP acquisition with both

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

arterial and ECG signals. In conclusion, this research establishes a potentially impactful and user-friendly approach for non-invasive JVP measurement. The proposed method eliminates the need for expensive equipment, complex infrastructure, and specialized personnel. This innovation holds promise for safer CVD diagnosis by minimizing risks associated with central venous line catheterization.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

## References

1. World Health Organization (WHO). Fact Sheets. Cardiovascular diseases (CVDs). Available from: [https://www.who.int/news-room/fact-sheets/detail/cardiovascular-diseases-\(cvds\)](https://www.who.int/news-room/fact-sheets/detail/cardiovascular-diseases-(cvds))
2. Constant J. Using internal jugular pulsations as a manometer for right atrial pressure measurements. *Cardiology*. 2000;93:26-30.
3. Applefeld MM. The jugular venous pressure and pulse contour. *Clinical Methods: The History, Physical, and Laboratory Examination*. Third edition. Butterworths; Boston, USA; 1990.
4. Irwin RS, Rippe JM, Celinski S, Snafu M. Central venous catheters. In: Irwin and Rippe's intensive care medicine. Lippincott Williams & Wilkins; Philadelphia, USA; 2008.
5. Menegatti E, Proto A, Paternò G, et al. The effect of submaximal exercise on jugular venous pulse assessed by a wearable cervical plethysmography system. *Diagnostics*. 2022;12:2407.
6. Tavoni V. Technical note for post processing of jugular venous pulse, central venous pressure and velocity trace. *Veins and Lymphatics*. 2020;9:8268.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

7. Zamboni P, Sisini F, Menegatti E, et al. Ultrasound monitoring of jugular venous pulse during space missions: proof of concept. *Ultrasound Med Biol*. 2018;44:726-33.
8. De Bonis P, Menegatti E, Cavallo MA, et al. JEDI (Jugular Entrapment, Dilated Ventricles, Intracranial hypertension) syndrome: a new clinical entity? A case report. *Acta Neurochir (Wien)*. 2019;161:1367-70.
9. Proto A, Conti D, Menegatti E, et al. Plethysmography system to monitor the jugular venous pulse: a feasibility study. *Diagnostics*. 2021;11:2390.
10. Alperin N, Lee SH, Sivaramakrishnan A, Hushek SG. Quantifying the effect of posture on intracranial physiology in humans by MRI flow studies. *Journal of Magnetic Resonance Imaging: an Official Journal of the International Society for Magnetic Resonance in Medicine*. 2005;22:591-6.
11. Zamboni P, Menegatti E, Pomidori L, et al. Does thoracic pump influence the cerebral venous return? *J Appl Physiol*. 2012;112:904-10.
12. Zamboni P, Menegatti E, Conforti P, et al. Assessment of cerebral venous return by a novel plethysmography method. *J Vasc Surg*. 2012;56:677-85.
13. Mohammed NY, Di Domenico G, Gambaccini M. Cerebral venous drainage through internal jugular vein. *Veins and Lymphatics*. 2019;8:8379.
14. Zamboni P, Tavoni V, Sisini F, et al. Venous compliance and clinical implications. *Veins and Lymphatics*. 2018;7:7367.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

15. Sisini F. Physical description of the blood flow from the internal jugular vein to the right atrium of the heart: new ultrasound application perspectives. 2016. Available from: <https://doi.org/10.48550/arXiv.1604.05171>
16. Sisini F, Tessari M, Gadda G, et al. An ultrasonographic technique to assess the jugular venous pulse: a proof of concept. *Ultrasound Med Biol*. 2015;41:1334-41.
17. Amelard R, Hughson RL, Greaves DK, et al. Non-contact hemodynamic imaging reveals the jugular venous pulse waveform. *Sci Rep*. 2017;7:40150.
18. Lam Po Tang EJ, HajiRassouliha A, Nash MP, et al. Non-contact quantification of jugular venous pulse waveforms from skin displacements. *Sci Rep*. 2018;8:17236.
19. García-López I, Rodríguez-Villegas E. Extracting the jugular venous pulse from anterior neck contact photoplethysmography. *Sci Rep*. 2020;10:3466.
20. Mari S, Pagani A, Valentini G, et al. Monitoring the cerebral venous drainage in space missions: the Drain Brain experiments of the Italian Space Agency. *Veins and Lymphatics*. 2023;12:11716.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*




**Figure 1.** Data acquisition setting.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

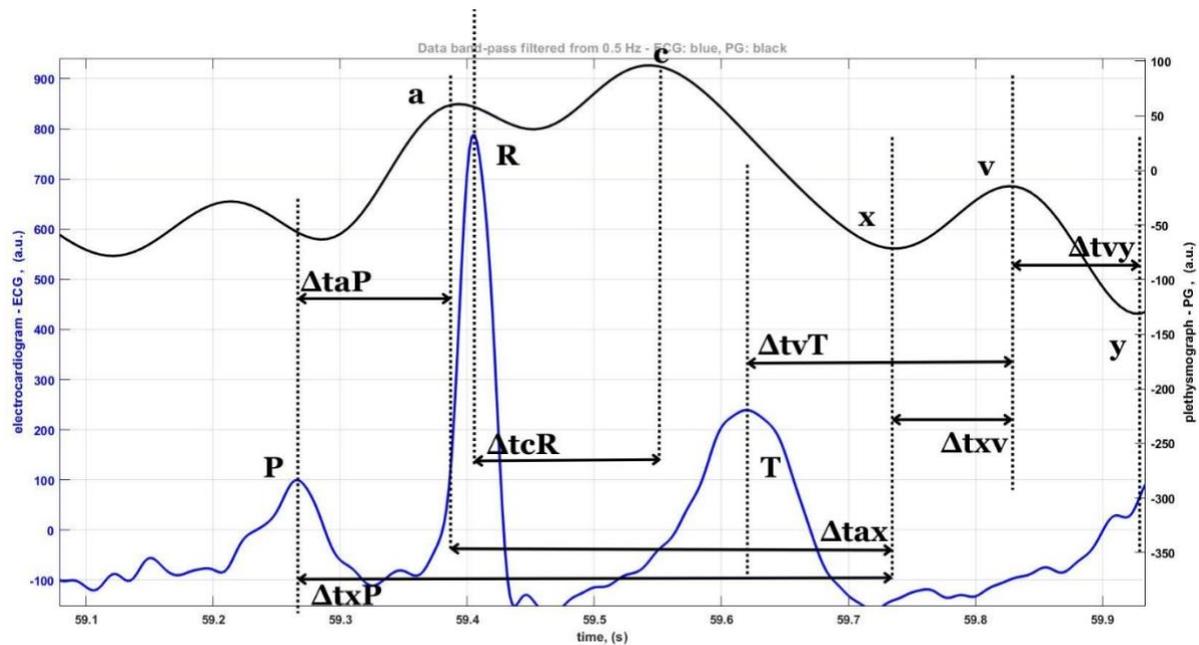


**Figure 2.** The Jugular Venous Pulse (JVP) signal (black), and the Electrocardiogram (ECG) signal (blue).

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

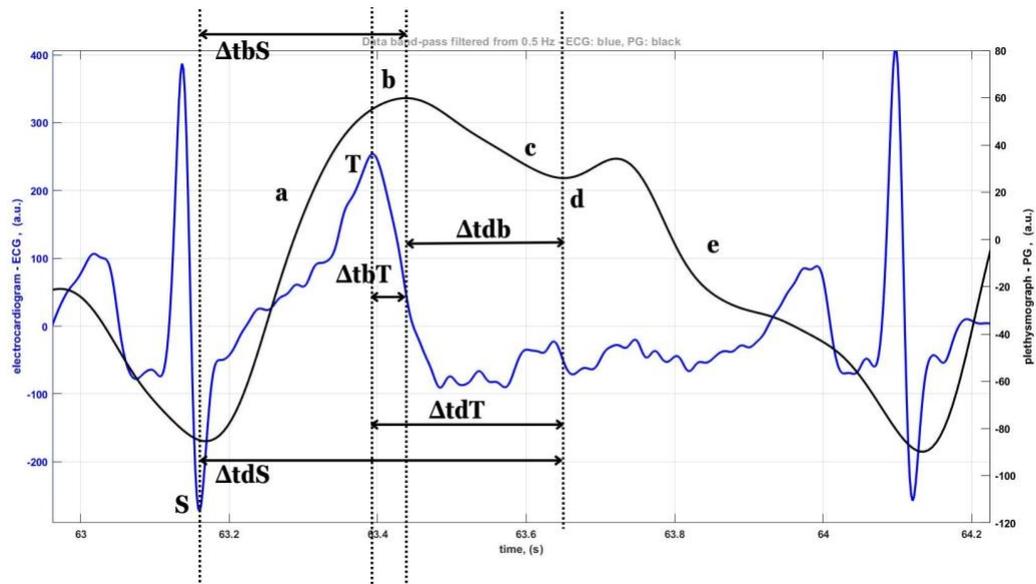


**Figure 3.** The Common Carotid Artery (CCA) signal (black), and the Electrocardiogram (ECG) signal (blue).

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

A)

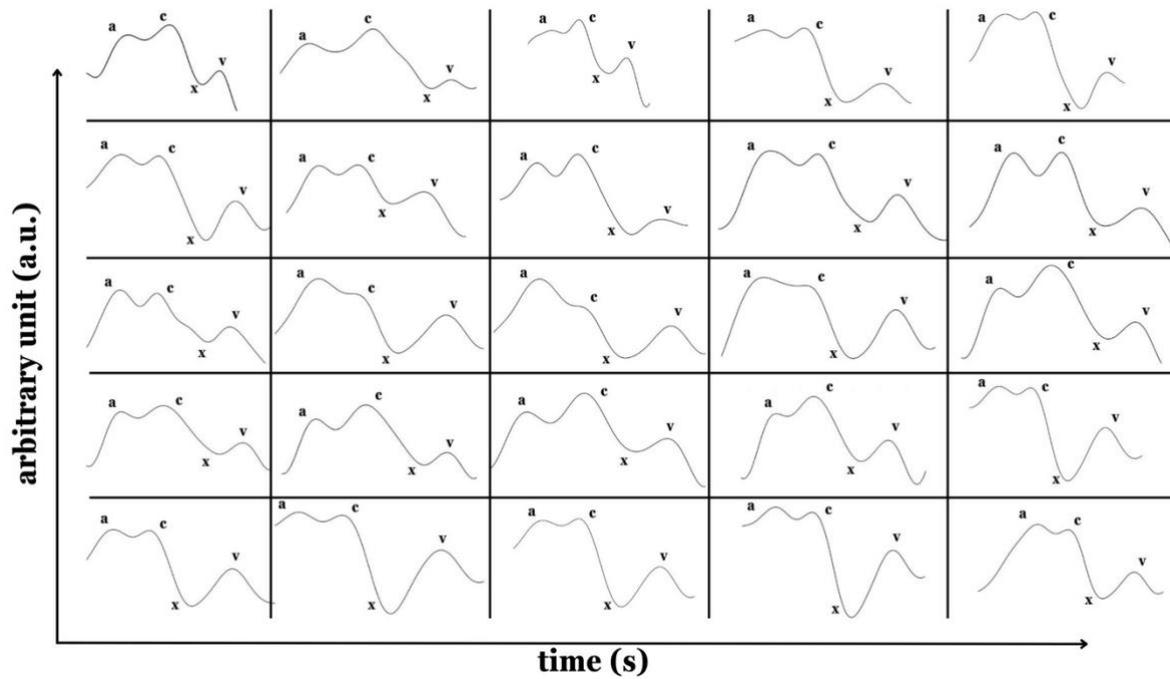


B)

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

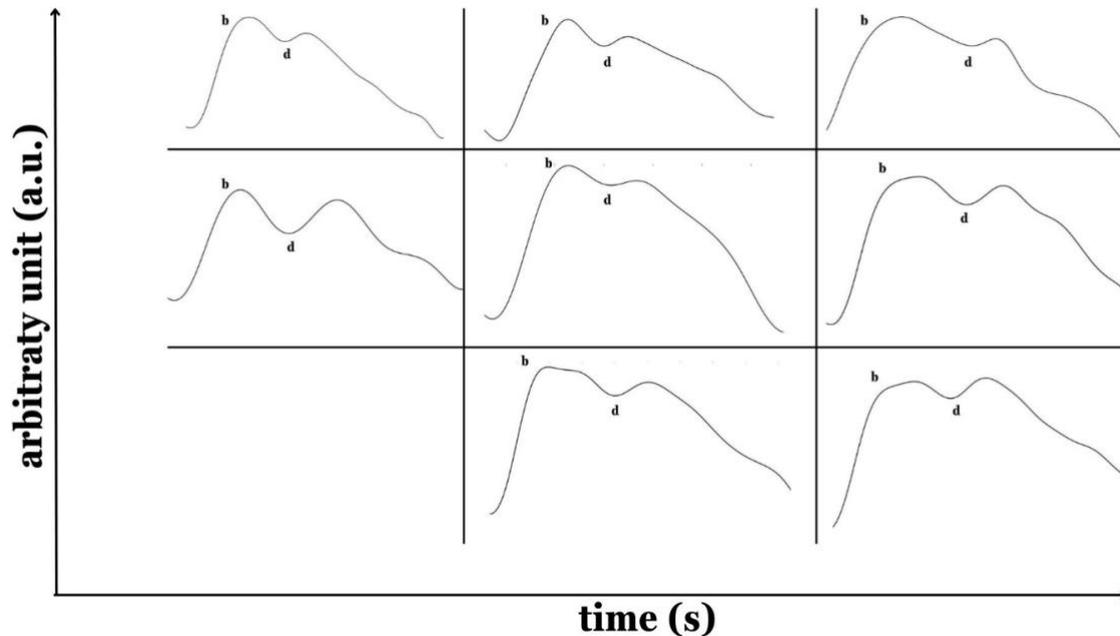

**Figure 4. A)** Example of a single cycle of Jugular Venous Pulse (JVP) signal extracted from each of the 26 subjects participating in the study. It is interesting to note the wide morphological variability of the signals. **B)** Example of a single Common Carotid Artery (CCA) signal cycle extracted from 8 subjects participating in the study. The y-axis units are arbitrary units because the data are filtered according to the procedure described in Materials and Methods. On the x-axis the units are seconds since these are time intervals.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*

**Table 1.** Data analysis: Fraction of the Cardiac Cycle (ccf) values, mean values, Standard Deviation (SD), and coefficient of variations values.

	$\Delta tcR$	$\Delta taP$	$\Delta txP$	$\Delta tvT$	$\Delta tyv$	$\Delta tvx$	$\Delta txa$
$\mu$ (ccf)	0,14	0,10	0,49	0,23	0,14	0,14	0,39
$\sigma$ (ccf)	0,04	0,04	0,12	0,06	0,03	0,03	0,09
<b>COV</b>	0,29	0,39	0,24	0,26	0,21	0,22	0,23
		$\Delta tdS$	$\Delta tdT$	$\Delta tdb$	$\Delta tbS$	$\Delta tbT$	
$\mu$ (ccf)		0,41	0,16	0,15	0,26	0,01	
$\sigma$ (ccf)		0,05	0,04	0,03	0,03	0,03	
<b>COV</b>		0,12	0,24	0,21	0,14	2,19	

The values reported are coherent with those reported by Tavoni,<sup>6</sup> in which the Jugular Venous Pulse (JVP) features were extracted using an Ultrasound (US) system.

*The publisher is not responsible for the content or functionality of any supporting information supplied by the authors. Any queries should be directed to the corresponding author for the article.*

*All claims expressed in this article are solely those of the authors and do not necessarily represent those of their affiliated organizations, or those of the publisher, the editors and the reviewers.*

*Any product that may be evaluated in this article or claim that may be made by its manufacturer is not guaranteed or endorsed by the publisher.*